



Automated Microtome Blade Changer  
Hendrick, Kendall B., et al  
Serial No. 09/844,833

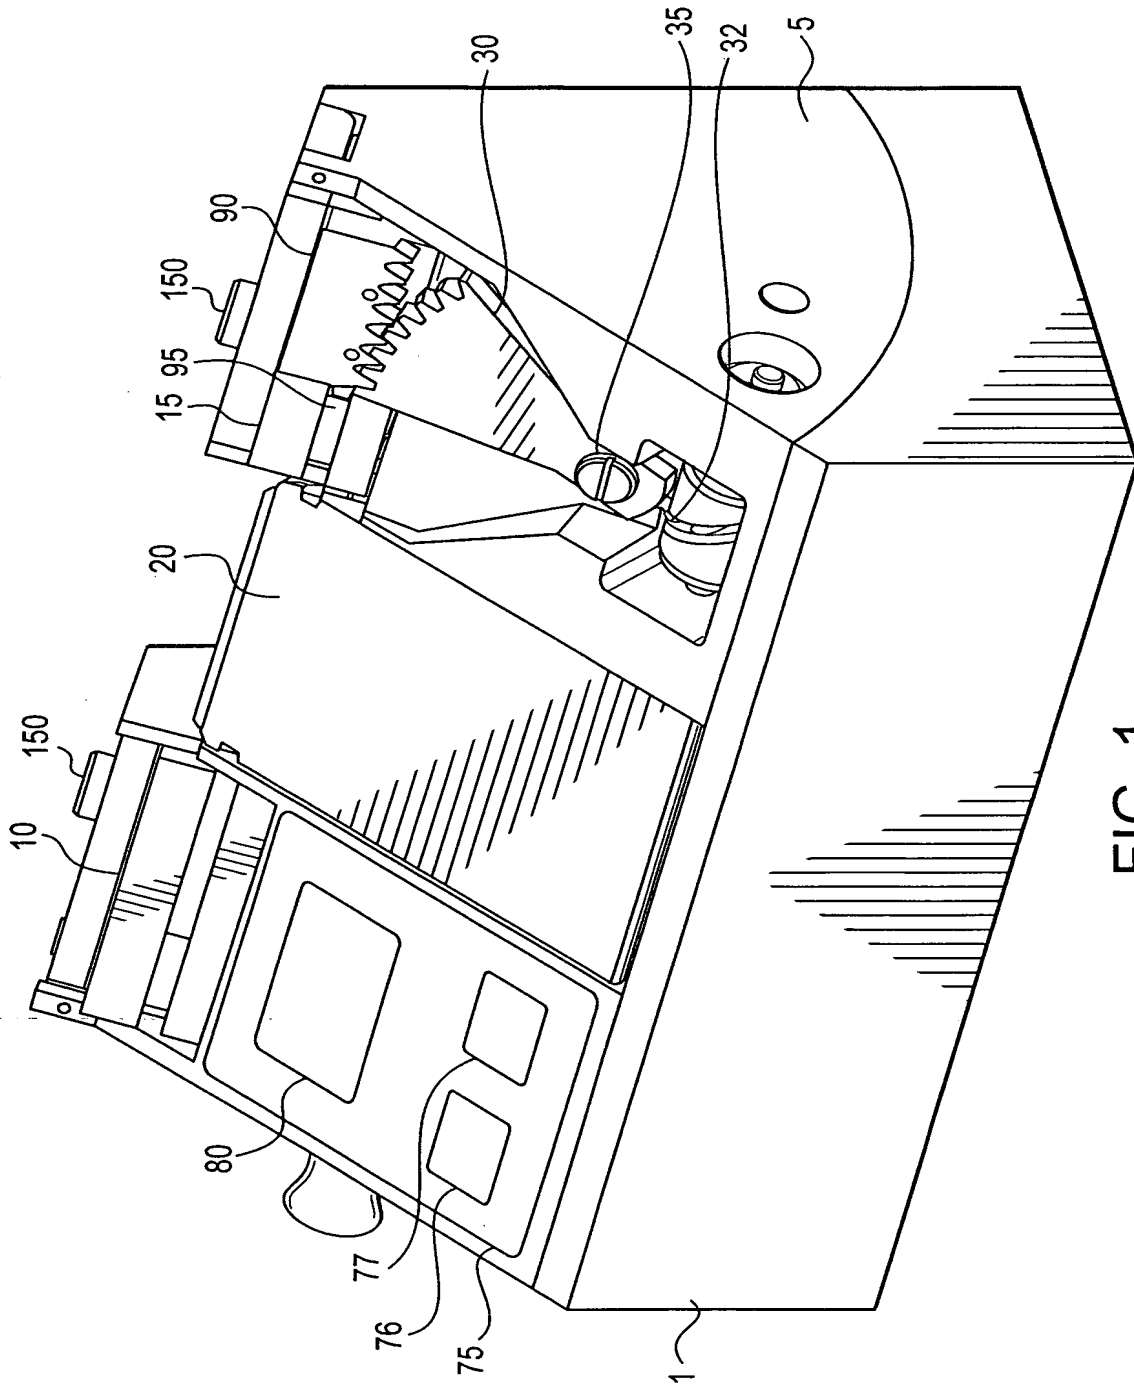


FIG. 1

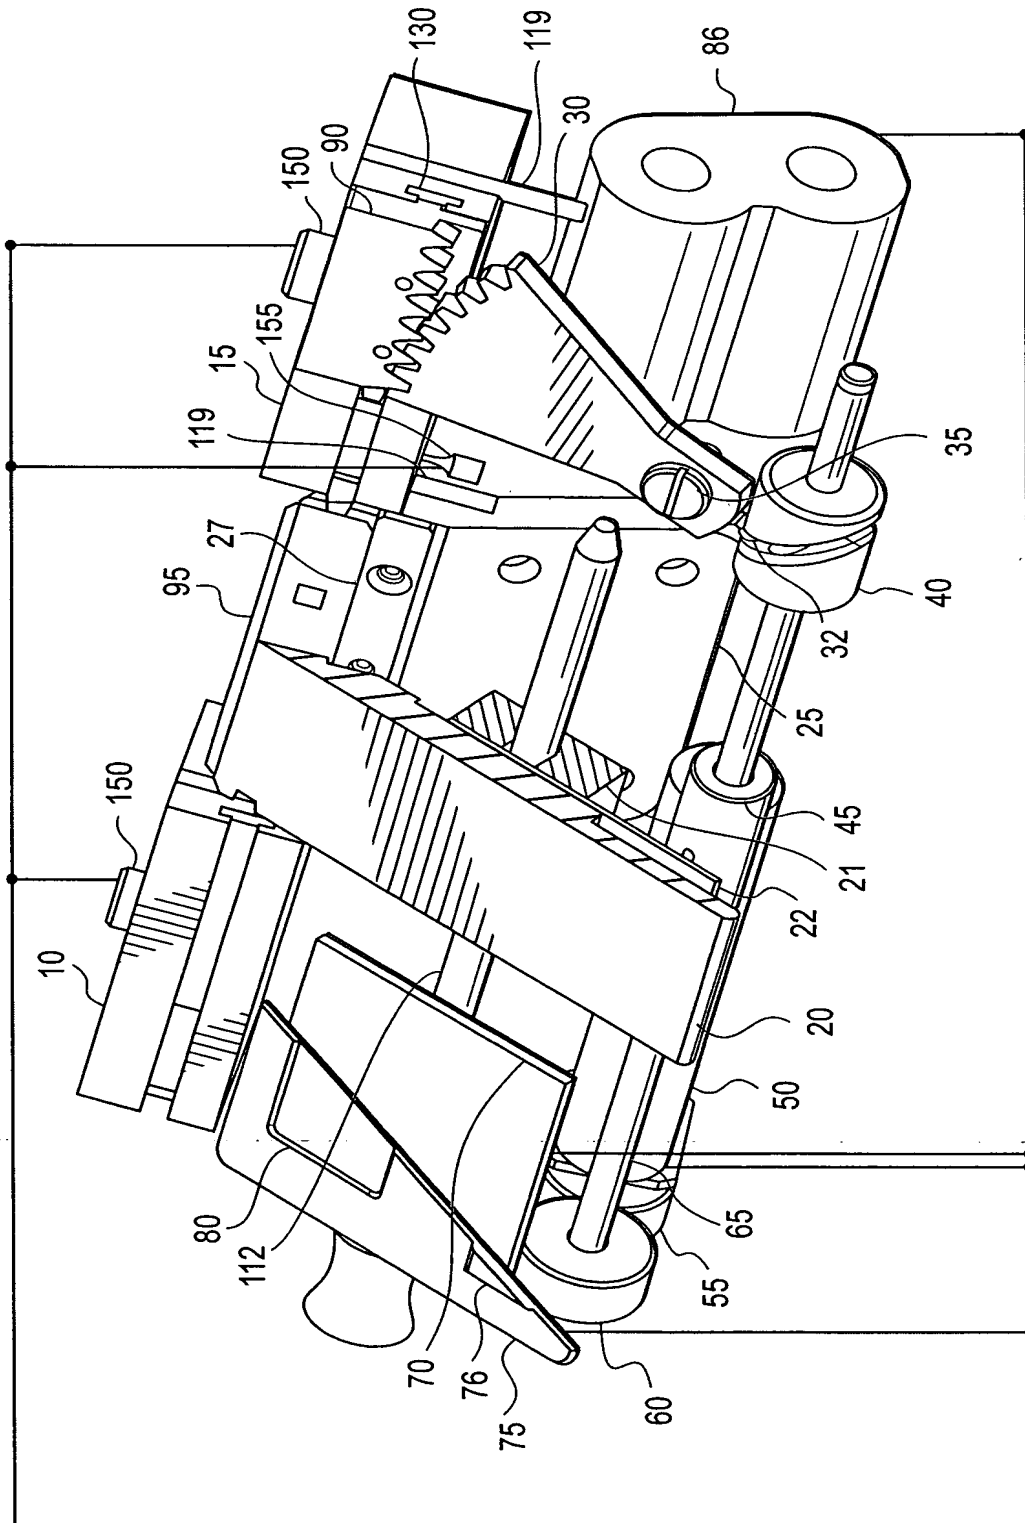


FIG. 2

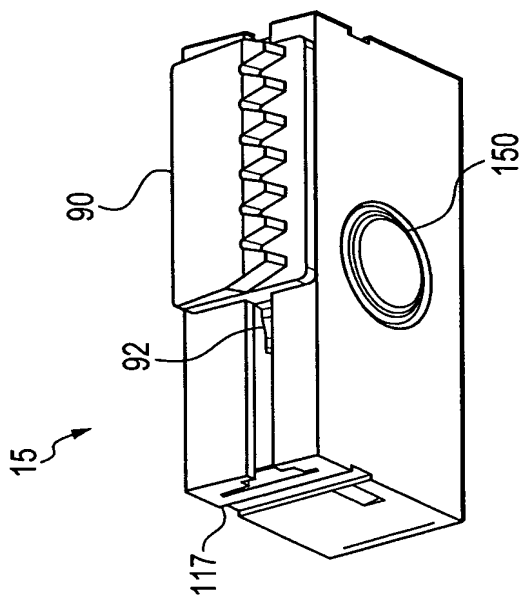


FIG. 3A

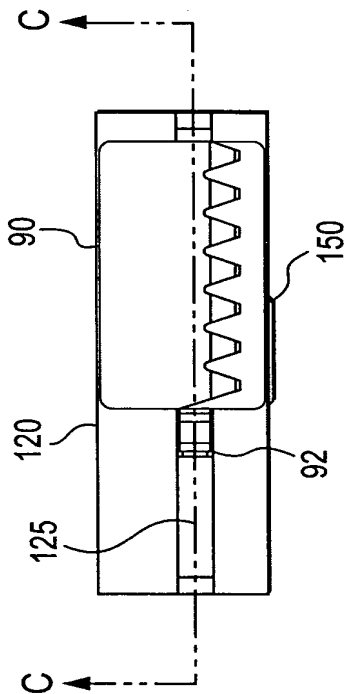


FIG. 3B

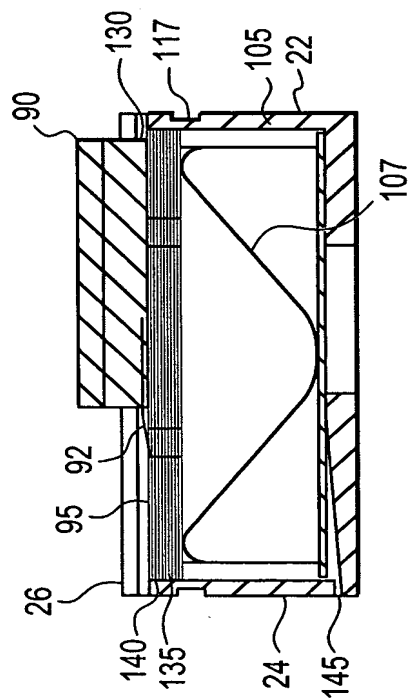


FIG. 3C

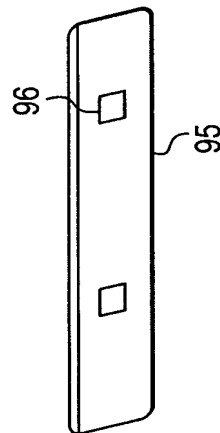


FIG. 3D

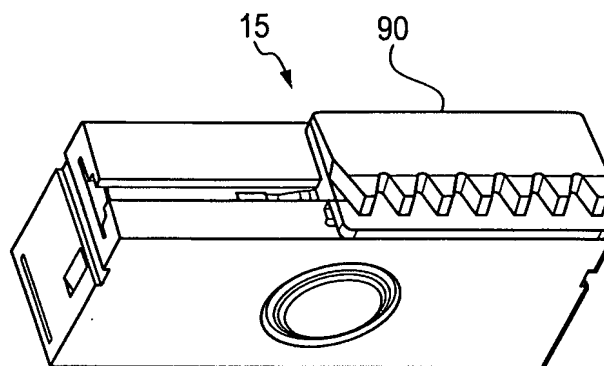


FIG. 4A

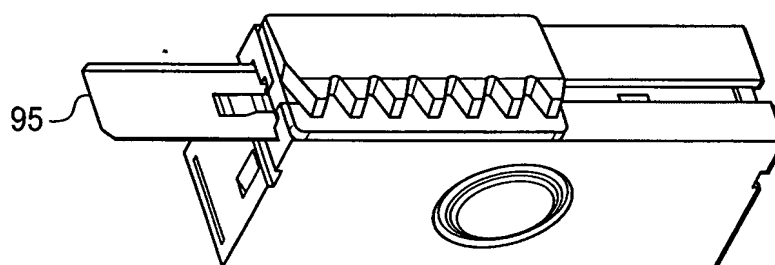


FIG. 4B

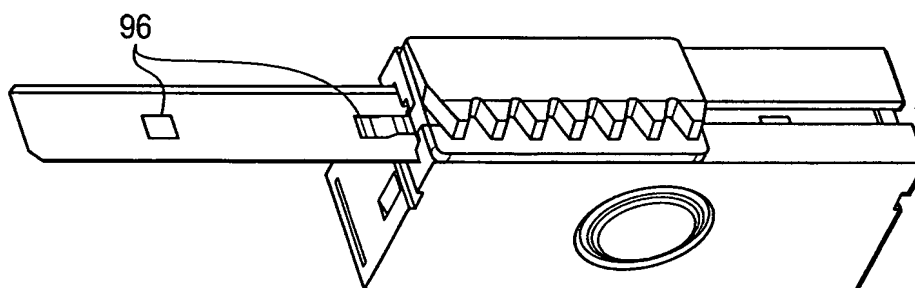


FIG. 4C

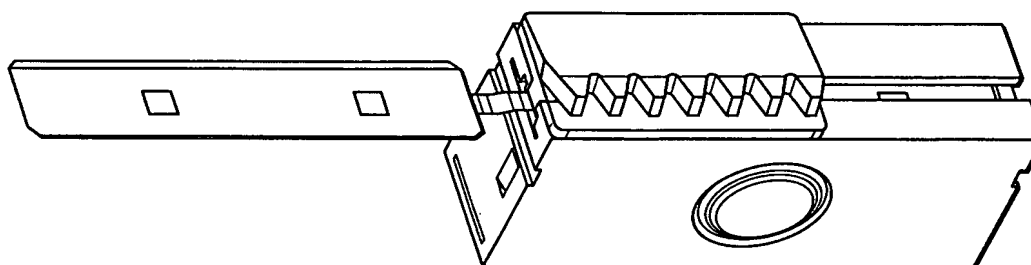
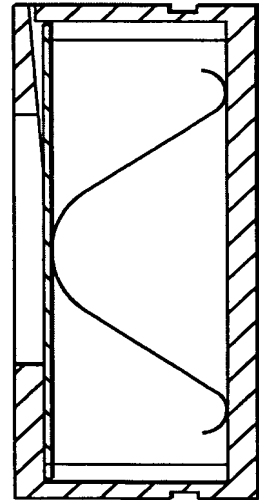
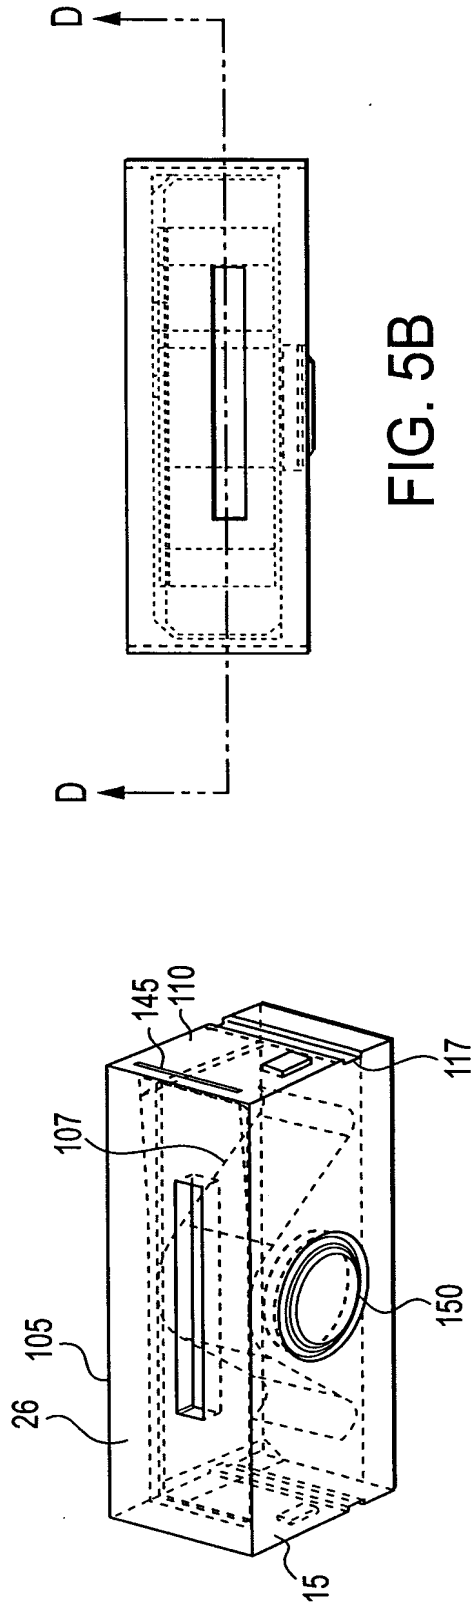


FIG. 4D



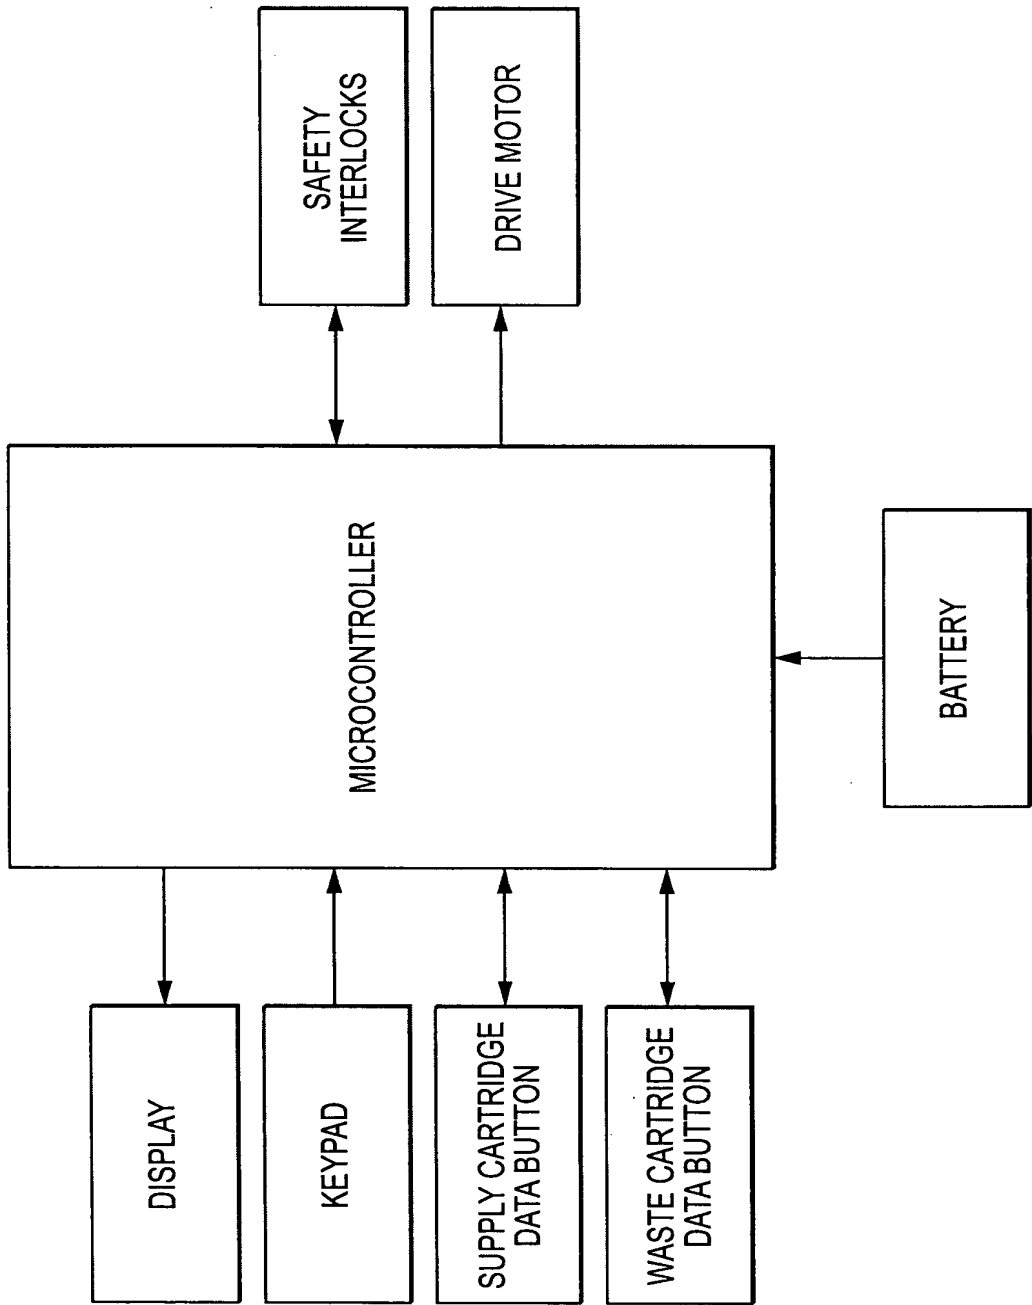


FIG. 6

**FIG. 7**

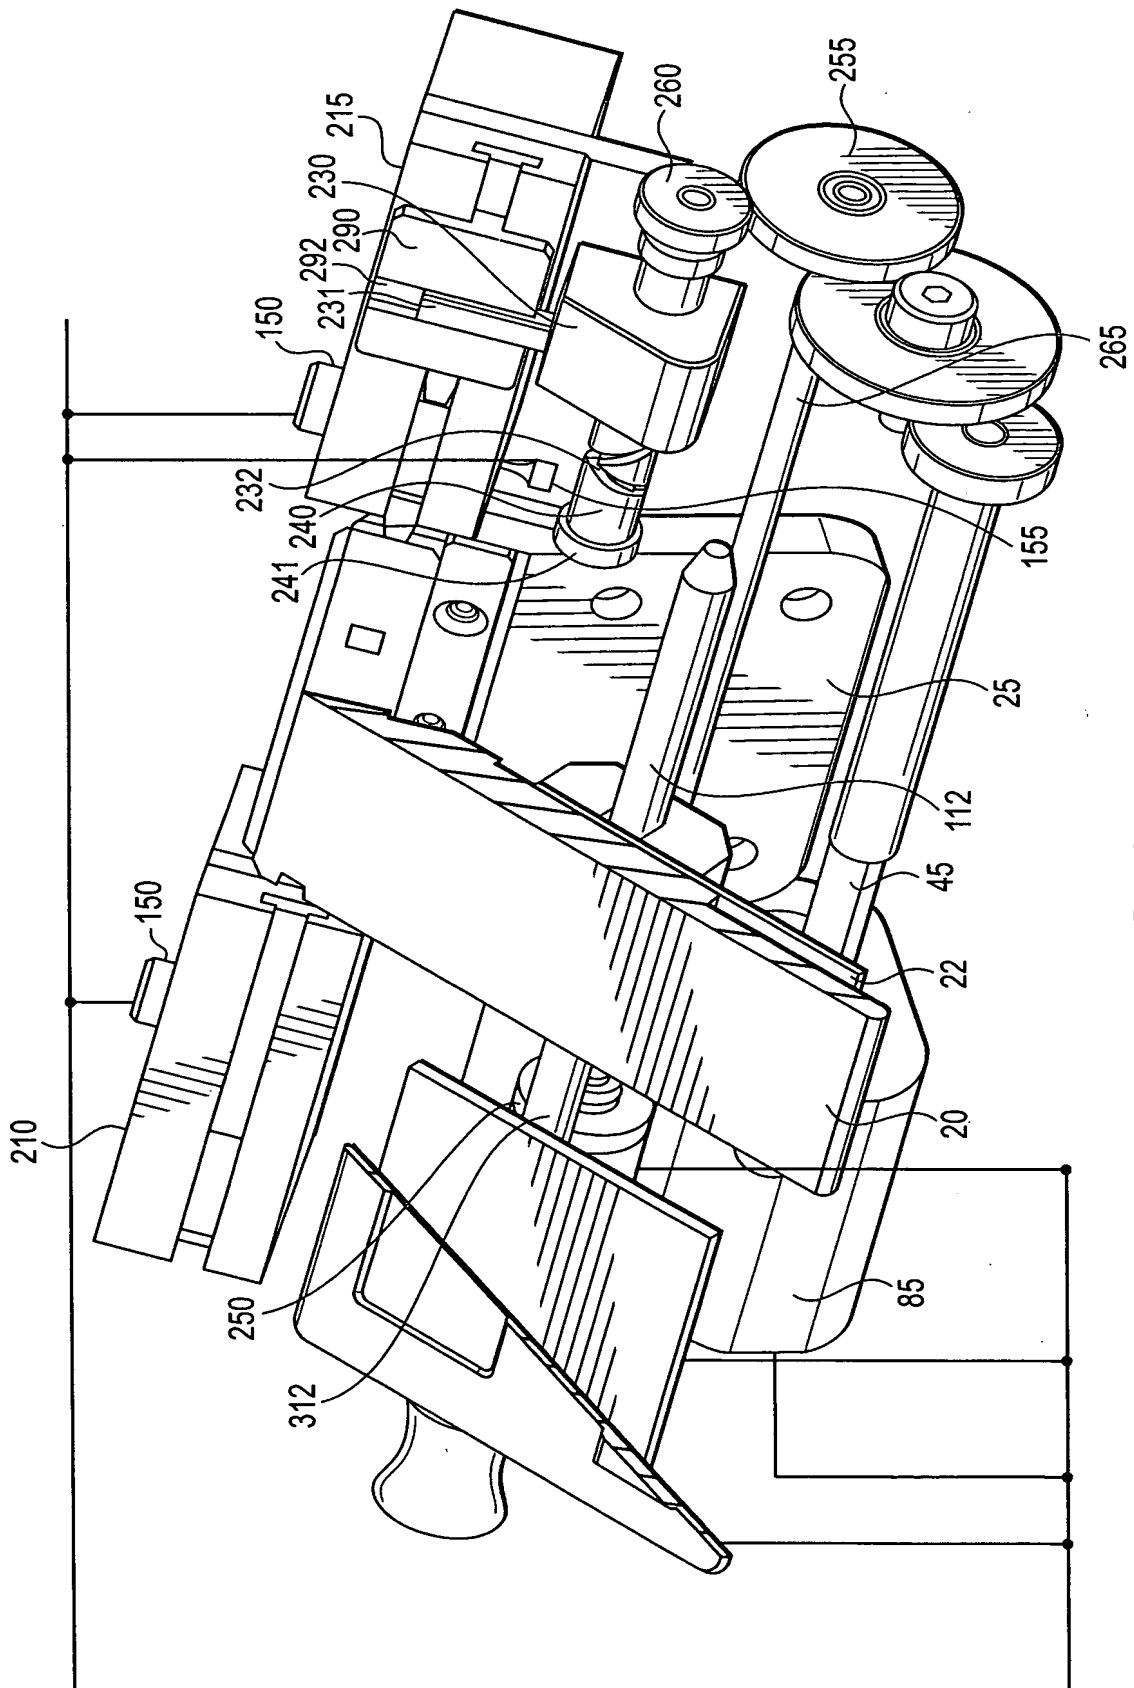


FIG. 8